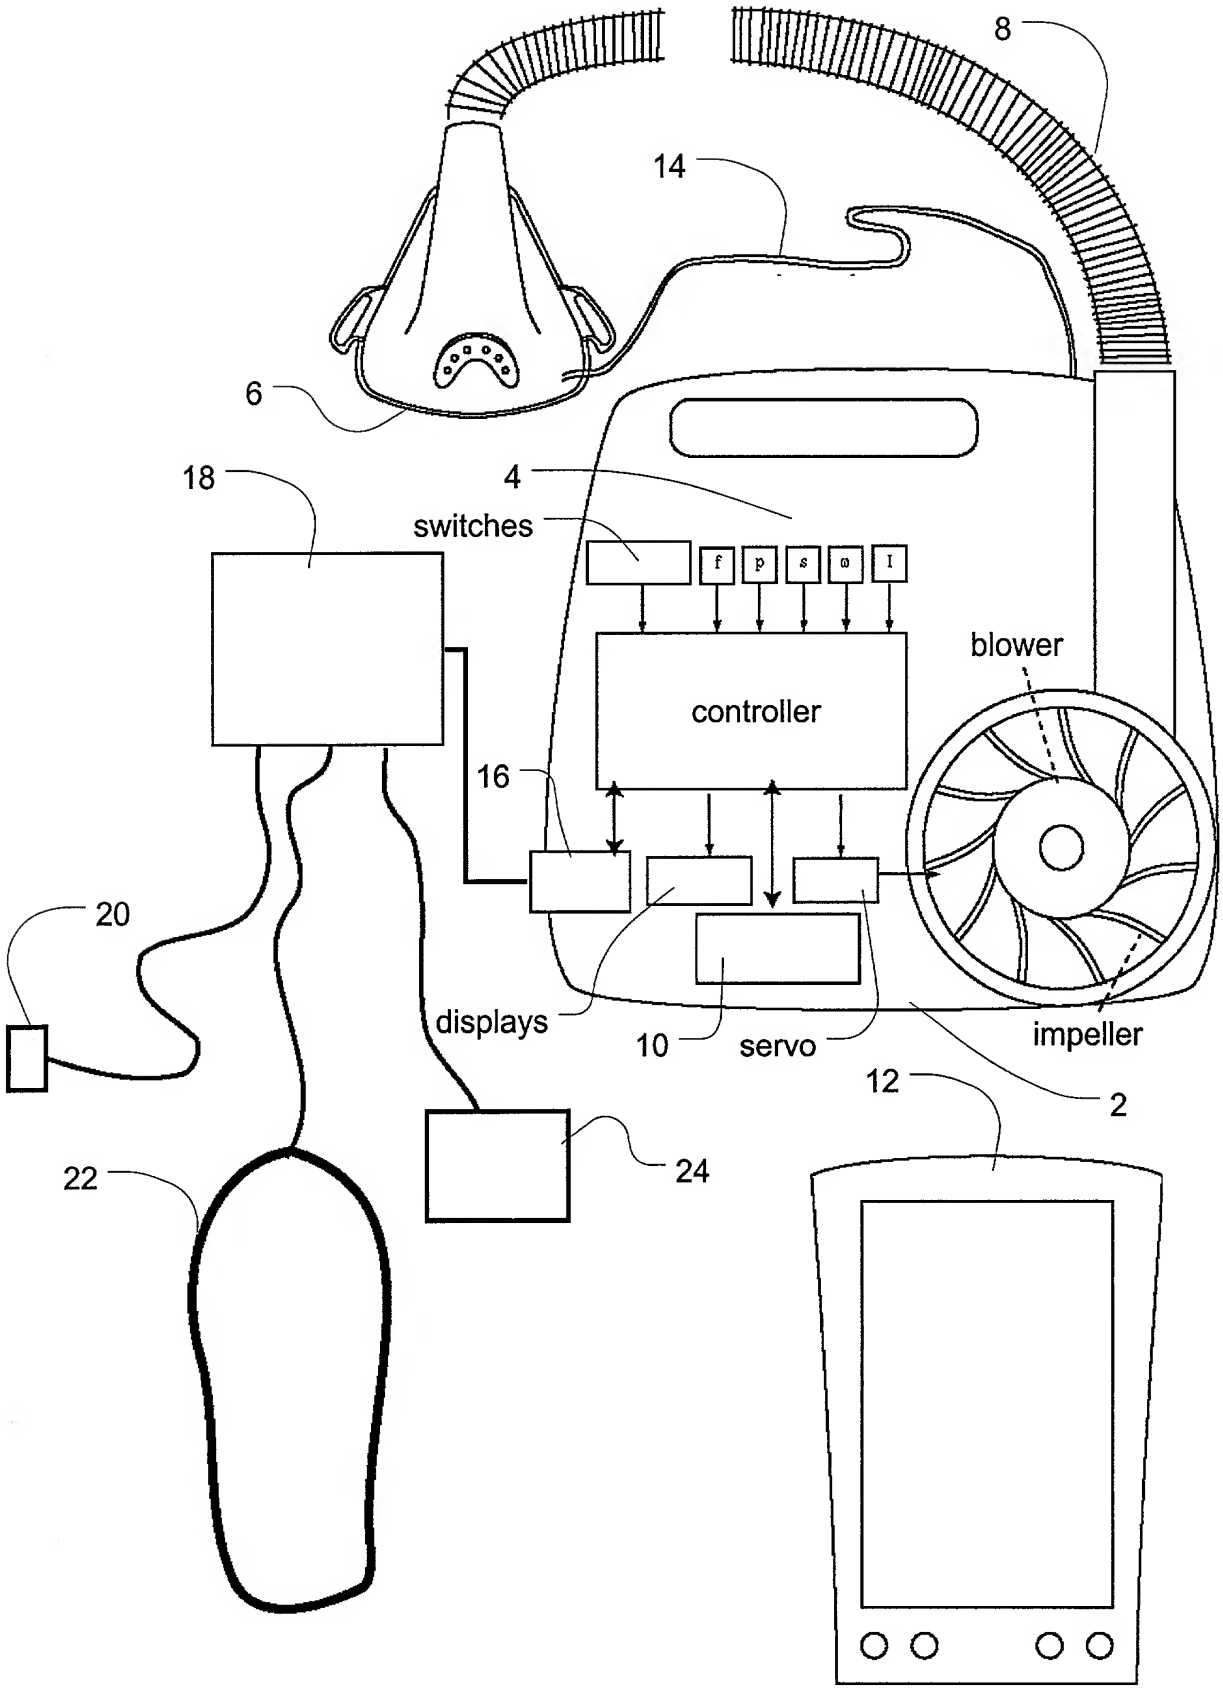
8
14
6
18
4
switches
f
p
s
a
I
blower
controller
16
20
displays
10
servo
impeller
2
12
24
22

Fig. 1

PATENT APPLICATION

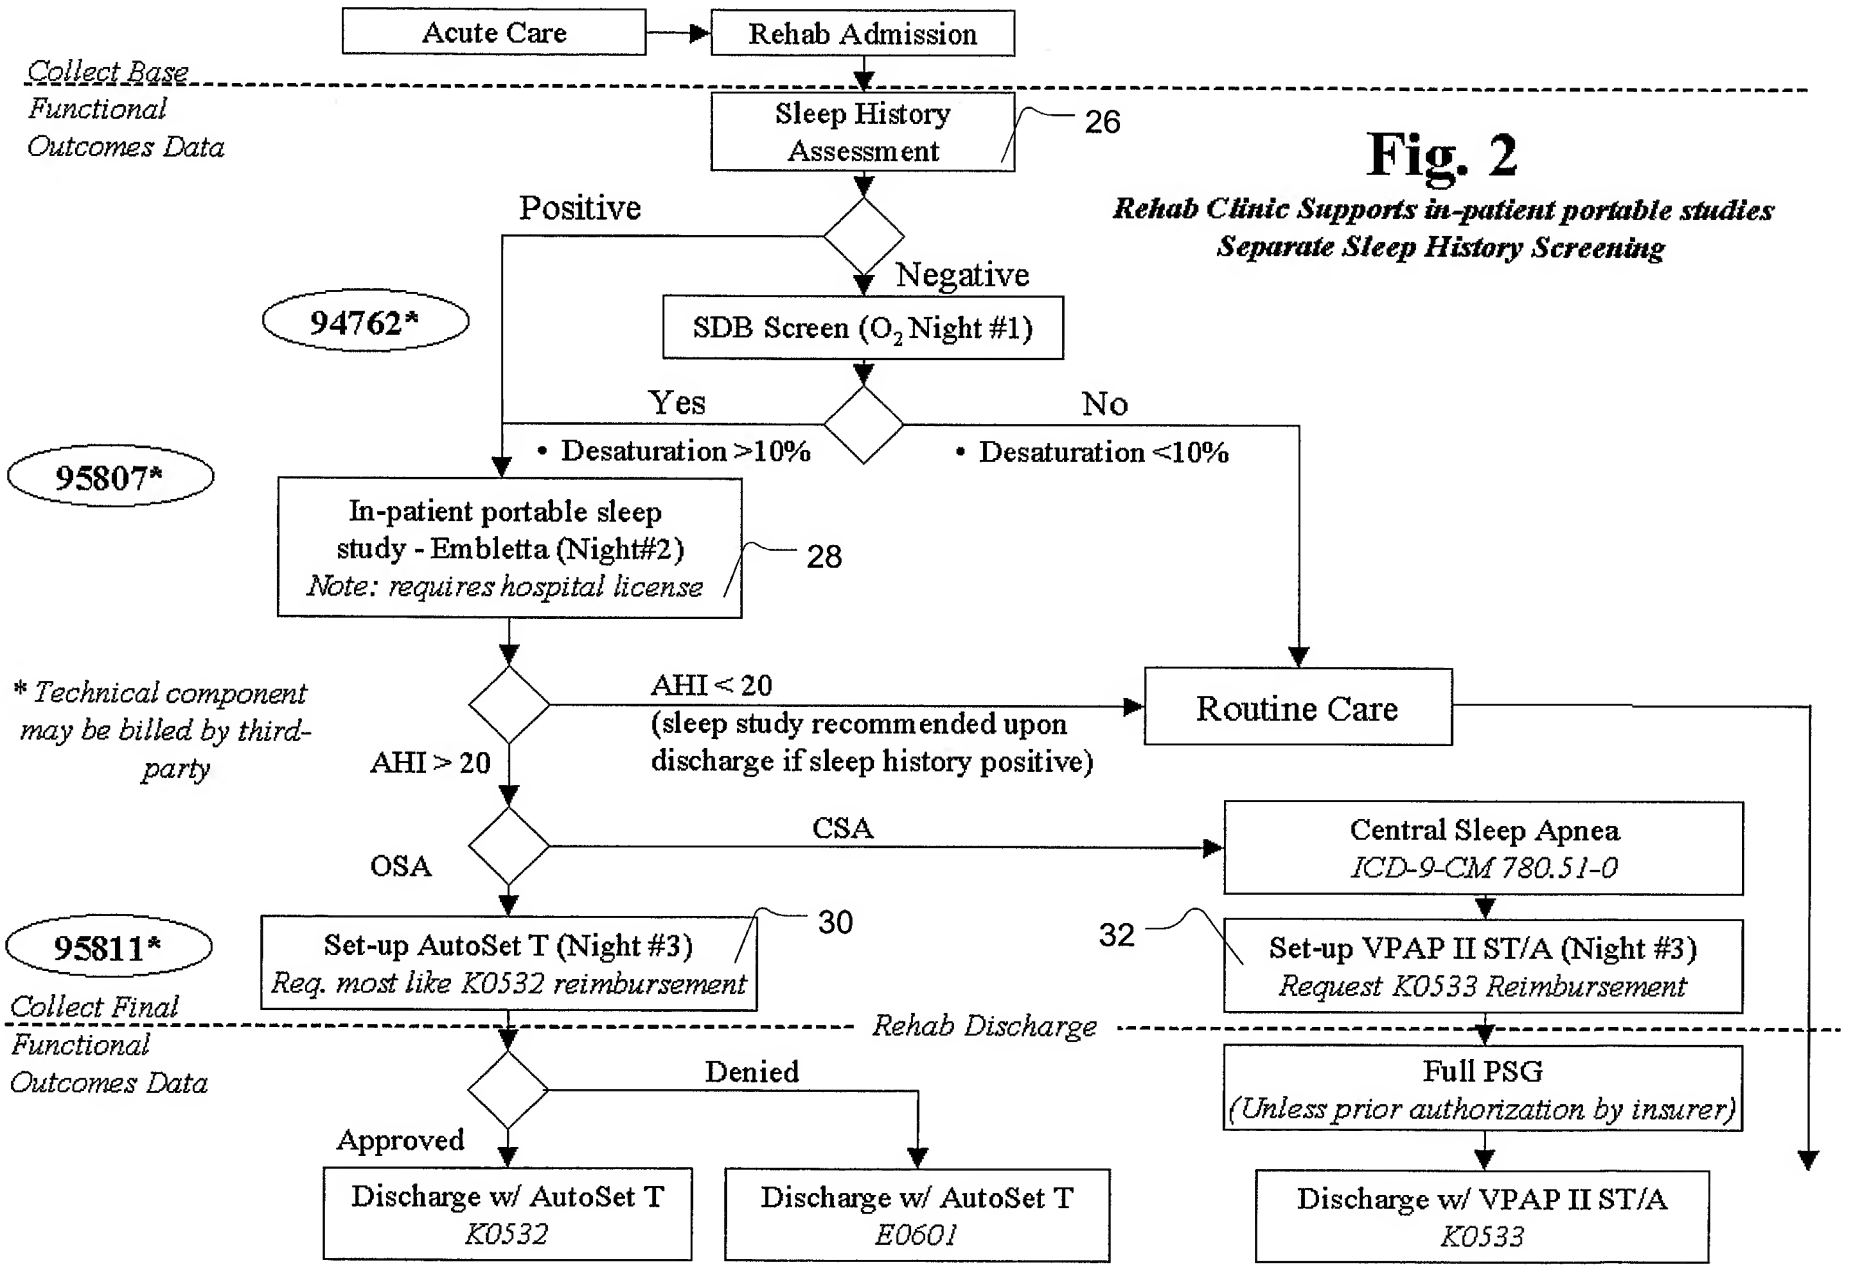

Fig. 2

Rehab Clinic Supports in-patient portable studies Separate Sleep History Screening

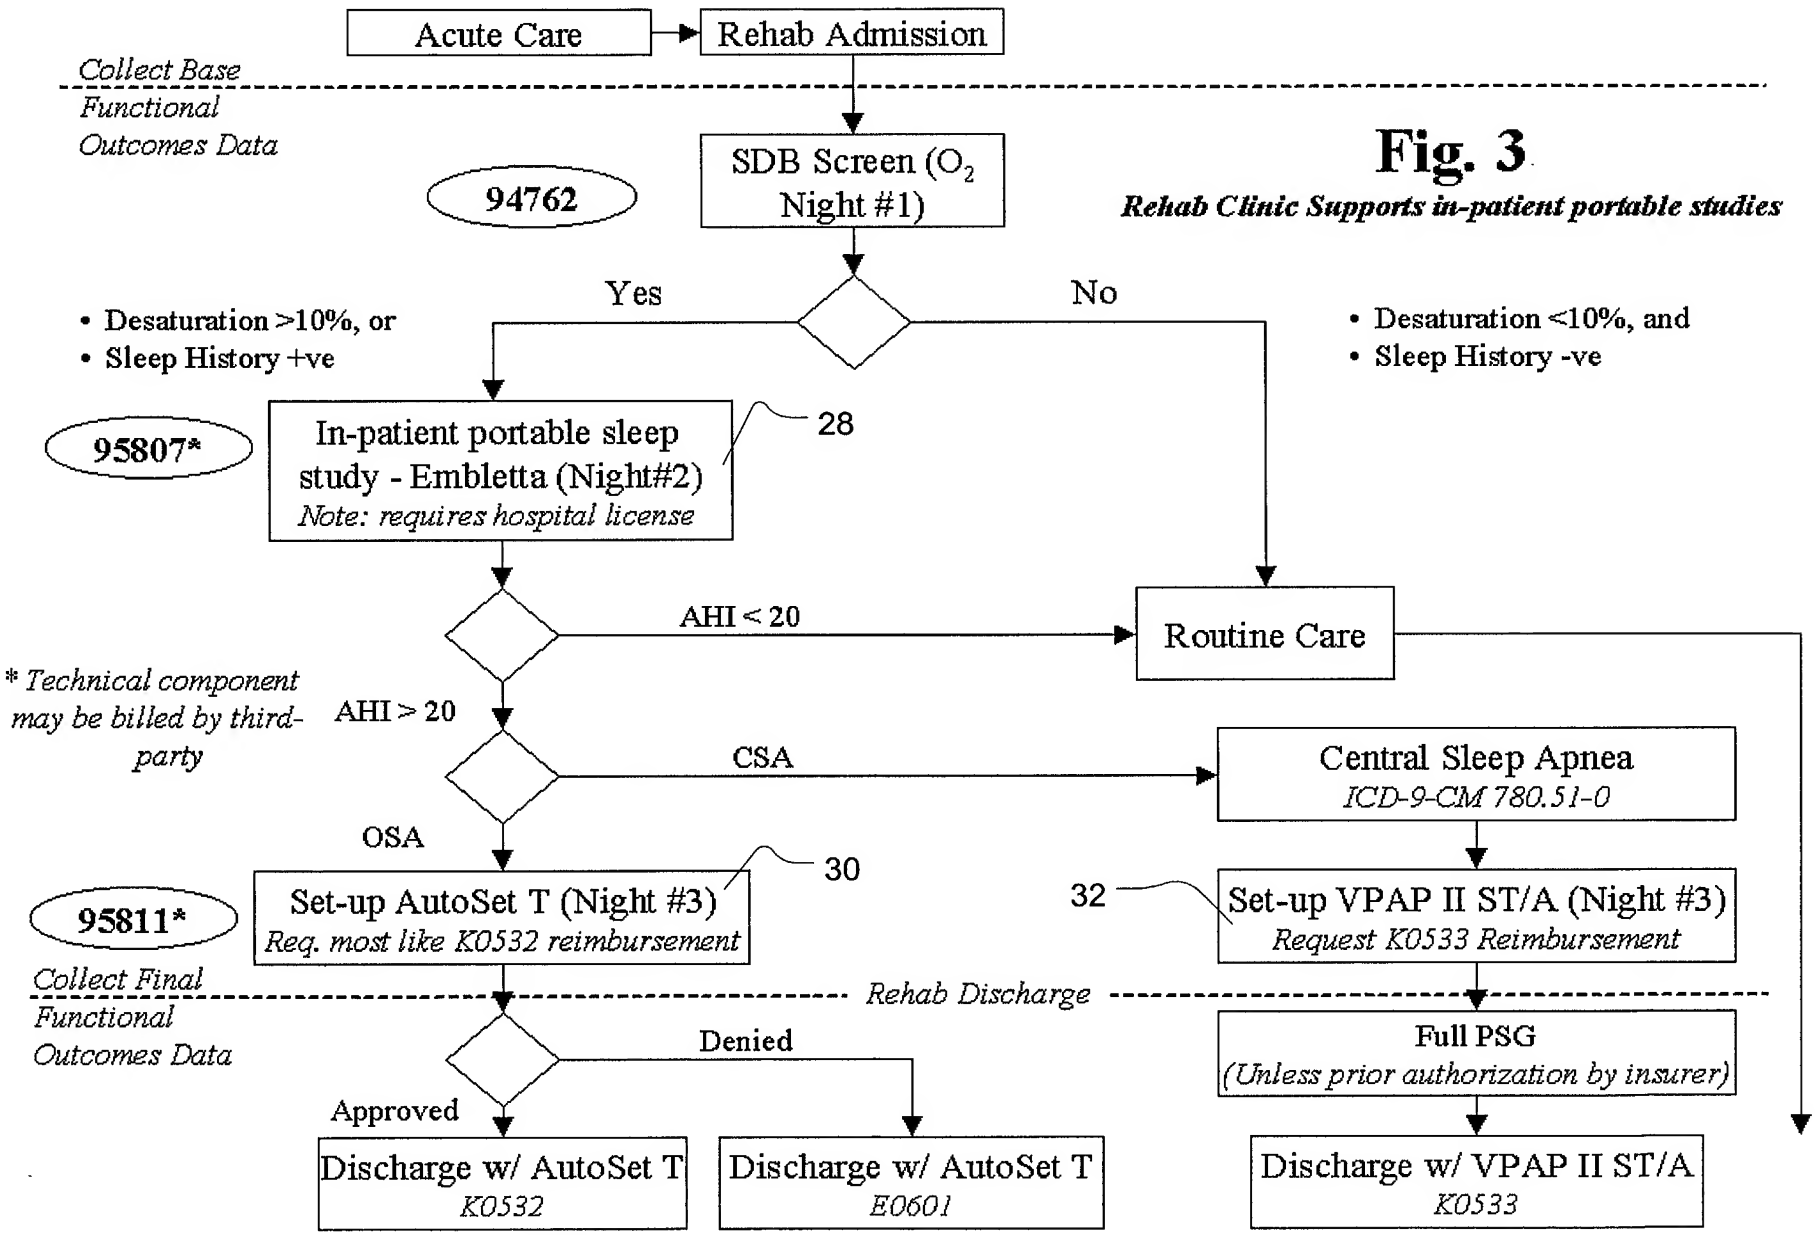

Fig. 3

Rehab Clinic Supports in-patient portable studies

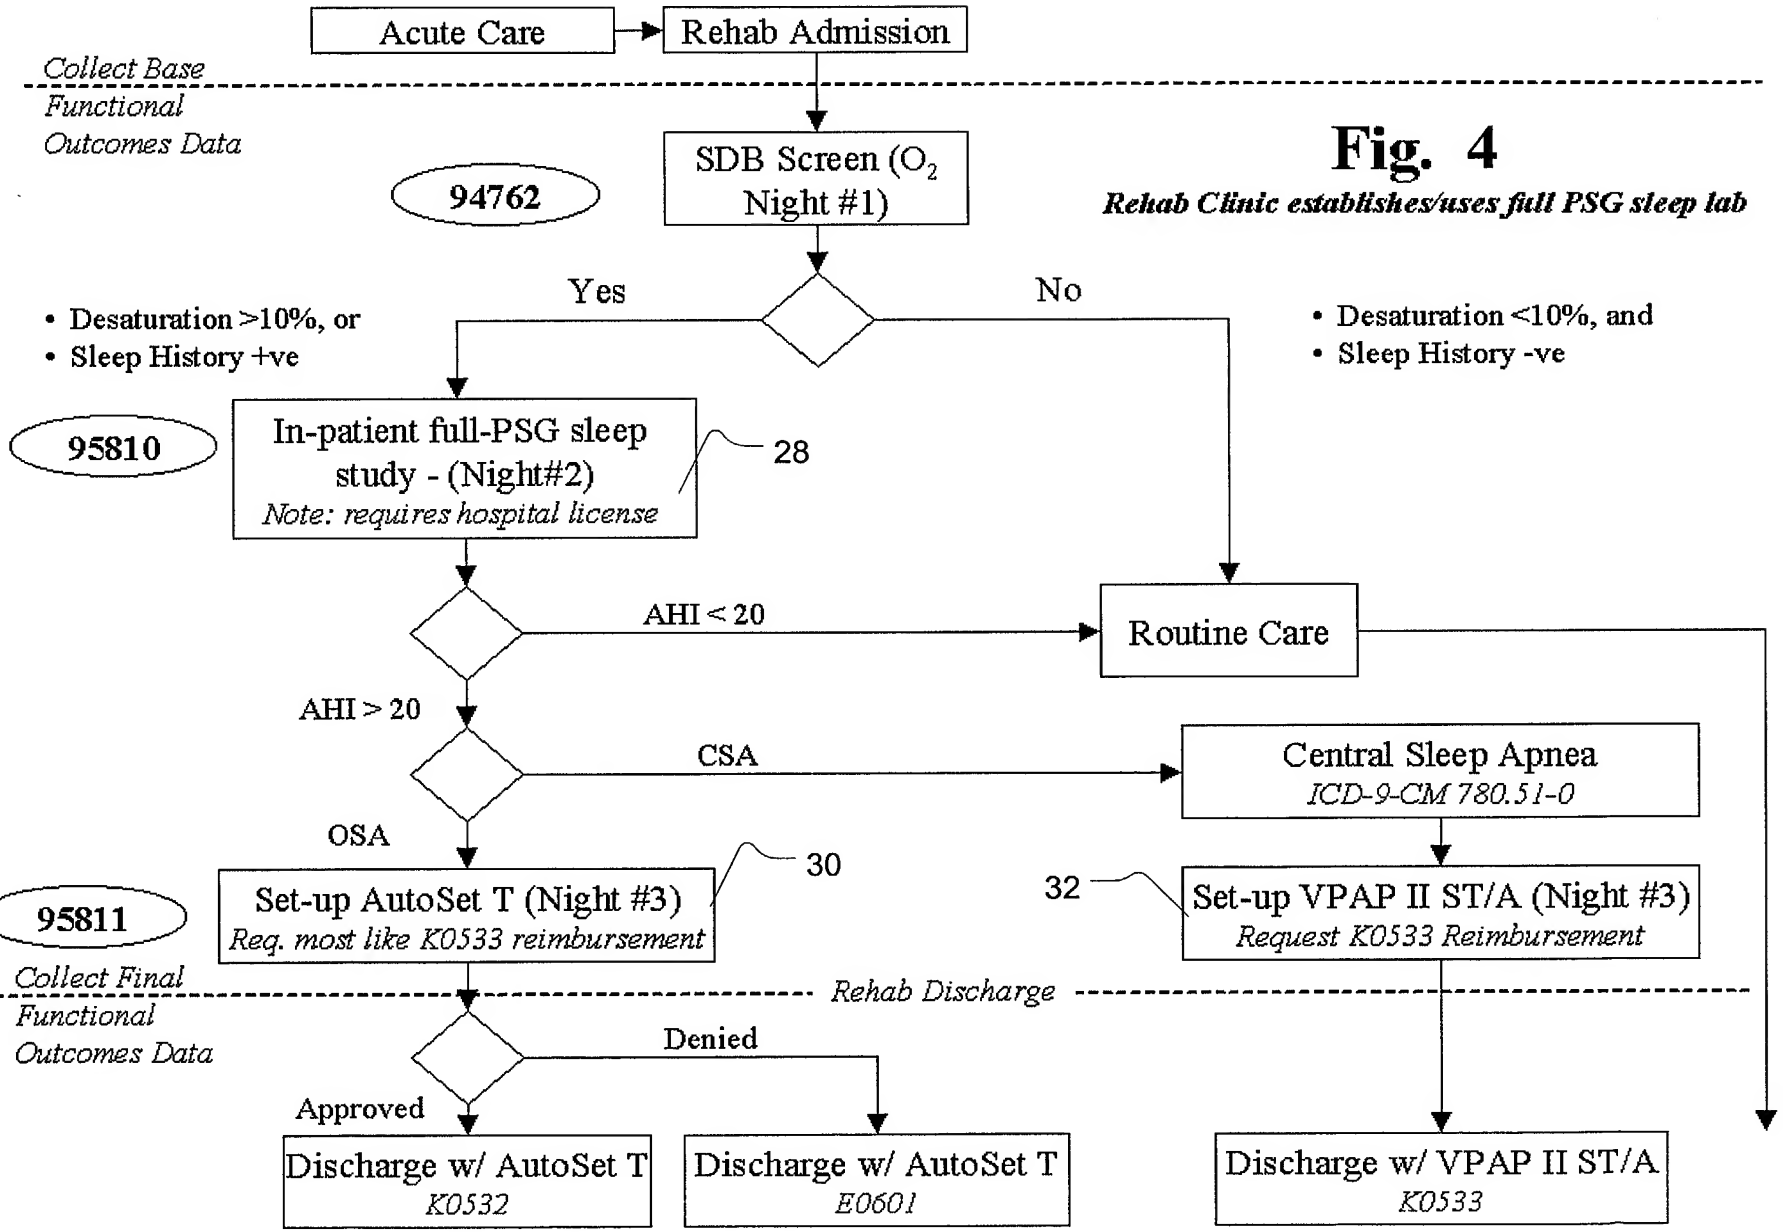

Fig. 4

Rehab Clinic establishes/uses full PSG sleep lab

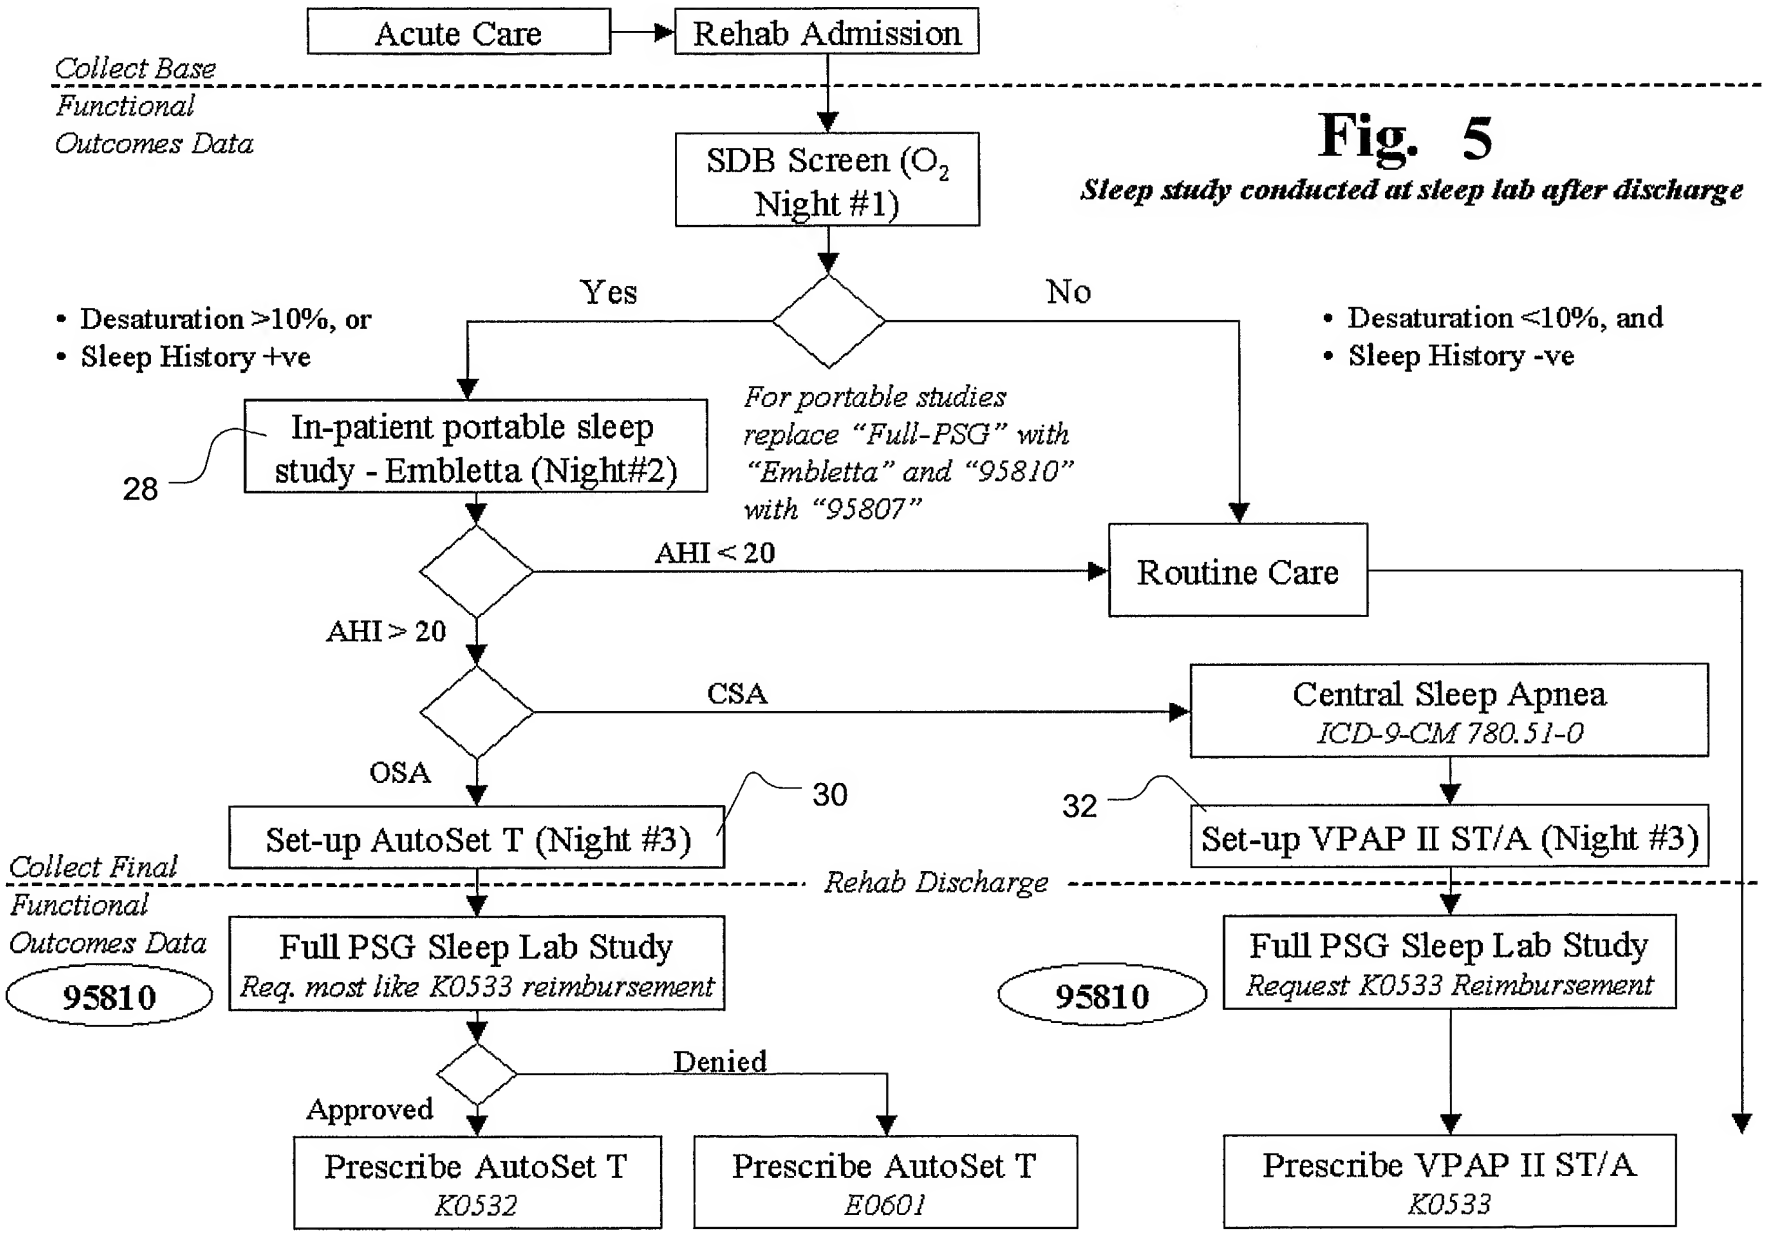

Fig. 5

Sleep study conducted at sleep lab after discharge

Fig. 6

Sleep study conducted at sleep lab prior to rehab

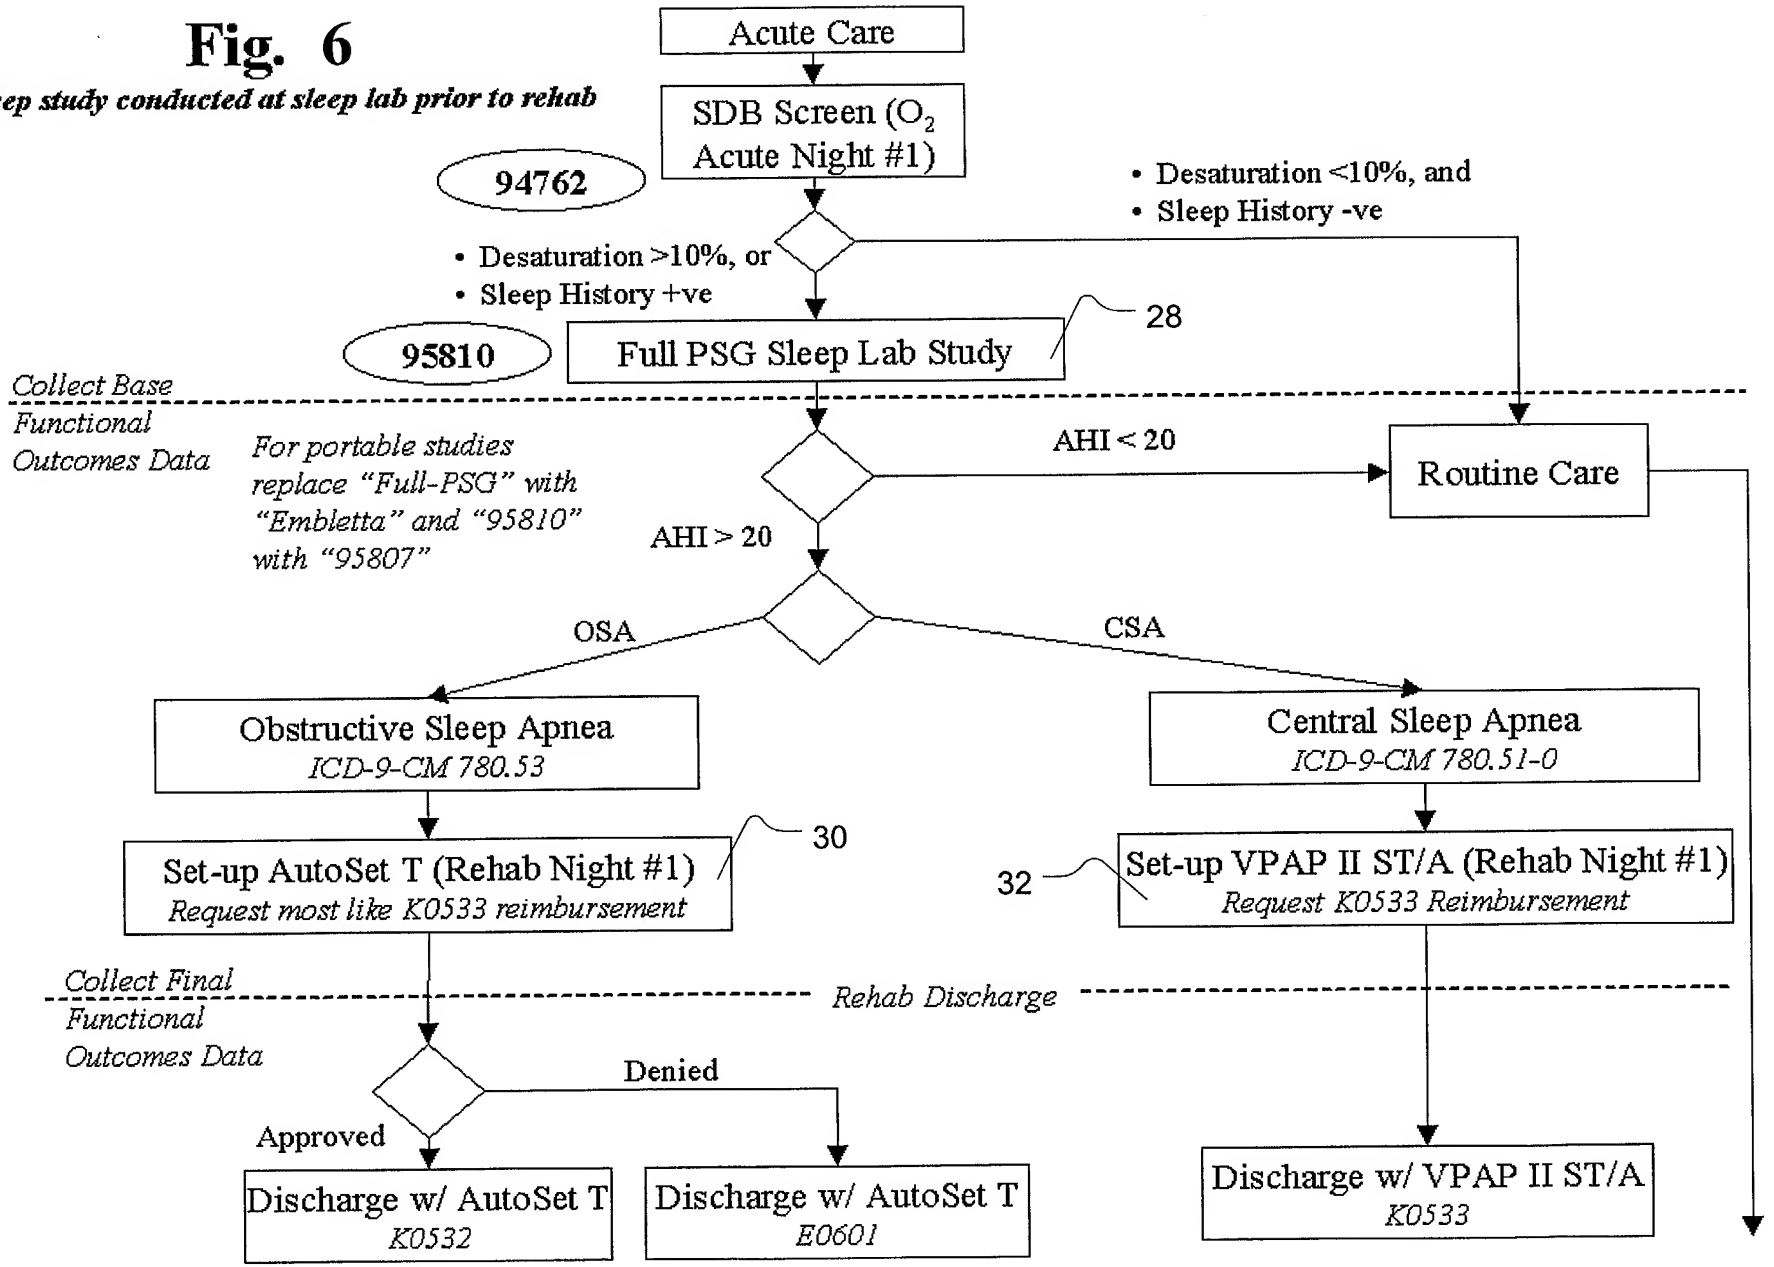
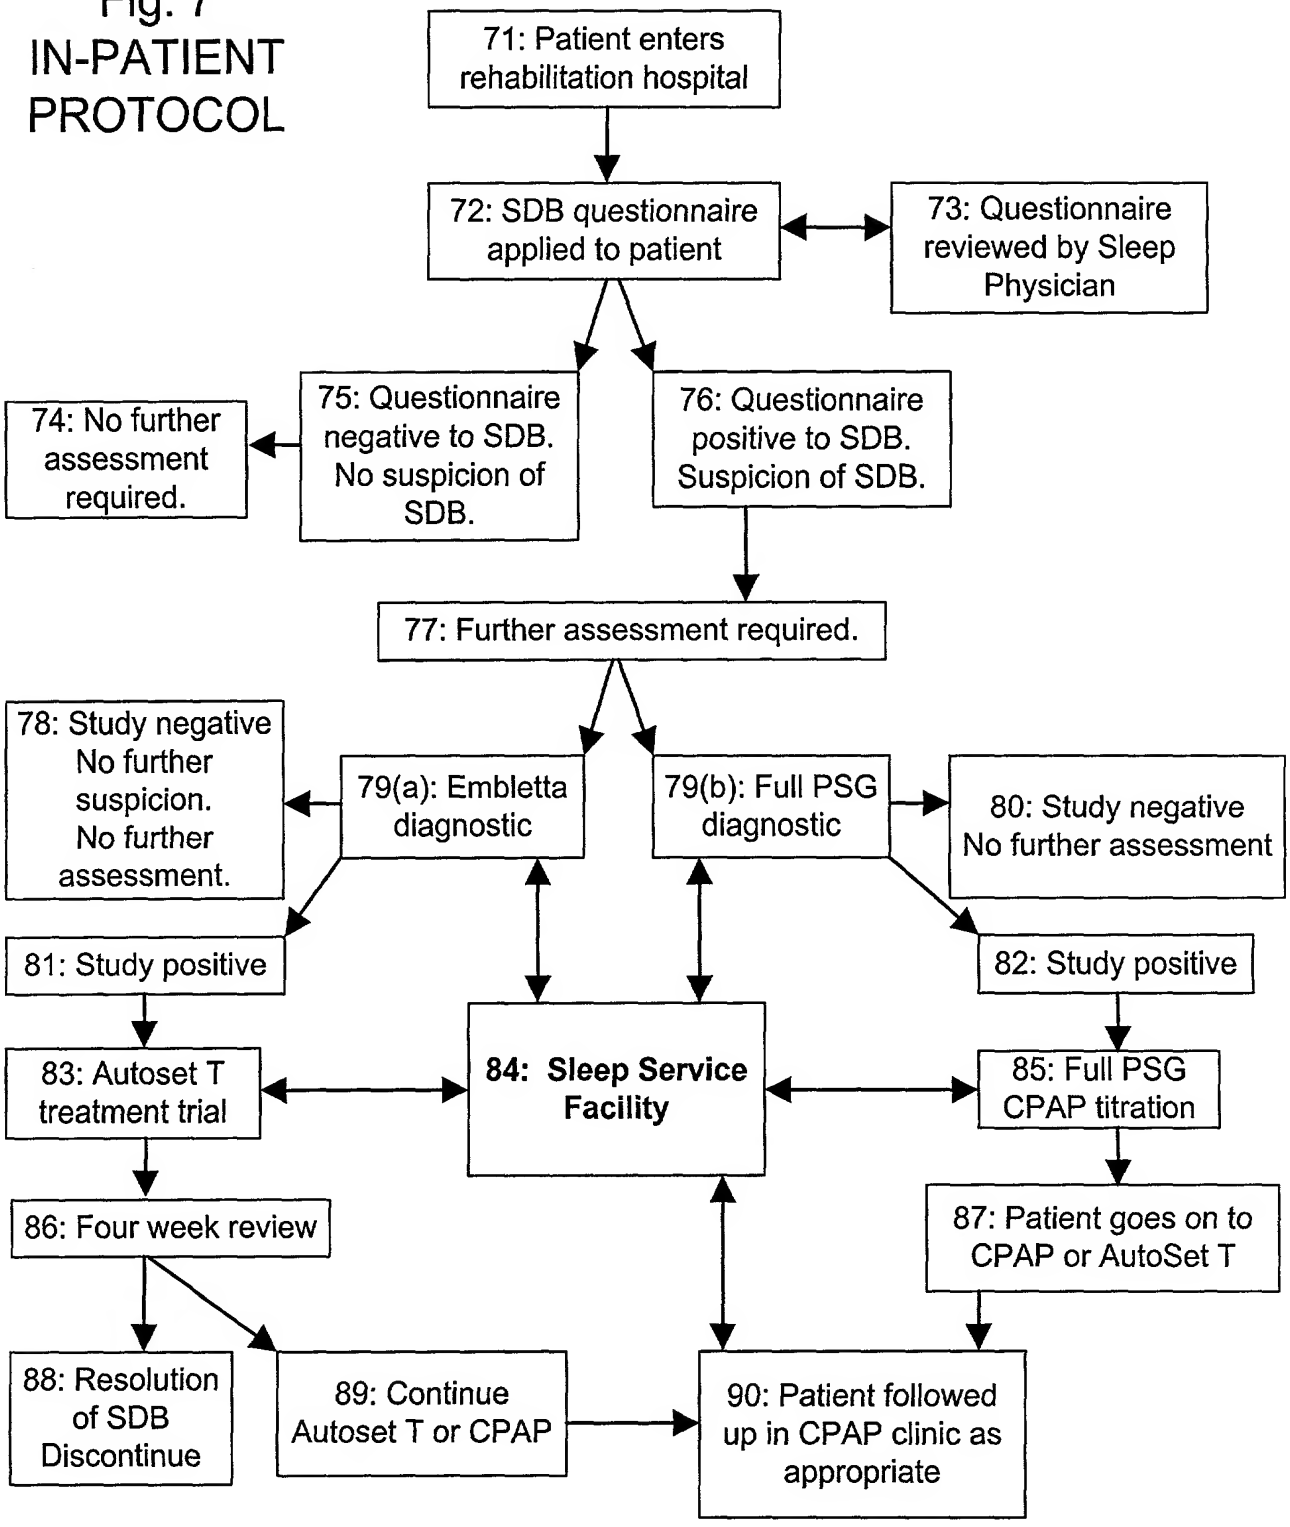
Fig. 7
IN-PATIENT
PROTOCOL